

Seta AvCount3 SA1100-0

Laboratory Particle Counter for Fuel, Lubes and Hydraulic Oils

ASTM D7619; ASTM D7647; ASTM D975; IP 565; Defence Standard 91-091; Defence Standard 91-86; IP PM FA; GOST 17216; ISO 4406; ISO 60970; NAS 1638; SAE 4059

- ISO 11171 calibration
- Cumulative counts/ml
- ISO 4406 cleanliness codes
- Colour touch screen
- Dilution ratio calculation
- Real time display of test progress
- User programmable
- LIMS, network and VNC connectivity
- Programmable alarm limits
- User and sample identification
- 14 embedded test methods
- Integral printer
- 500,000 test memory
- In-field verification and calibration



Fuels • Hydraulic Oil • Light Lubricants



Seta AvCount3

Laboratory Particle Counter for Fuel, Lubes and Hydraulic Oils

ASTM D7619; ATM D7647; ASTM D975; IP 565; Defence Standard 91-091; Defence Standard 91-86; IP PM FA; GOST 17216; ISO 4406; ISO 60970; NAS 1638; SAE 4059

8" LCD Power saving touchscreen mode Outlet Inlet avcounta USB port Internal printer

AvCount3 Particle Counter


The AvCount3 is a compact bench-top automatic particle counter, used to measure the size and distribution of particles and water droplets in light and middle distillate fuels, including aviation fuel and kerosine, biodiesel, low viscosity oils and hydraulic oils.

The test process is fully automated. Having prepared your sample in accordance with method instructions, simply insert the metal dip tube into the sample container, select a test method and initiate the test, the test proceeds without any further operator intervention.

Operator Interface

Start of Test					
Operator:				14	
Sample:					
Method:	ISO 4406				C
		1 measureme	nt	Flush	
Dilution:	0%	No multiplier	Sample: 200 ml Diluent: None		
Comment:					
Press ► to start	21-Jun-2021 16:33:01	F			

> Enter operator and sample details, select method, press



> Test begins, instrument sequences are detailed

> Final result displays either numerically or graphically

Result Display

6.0

14.0

25.0 38.0 70.3

Corrected Raw data

1144.9

65.8

10.4

20/17/13

DAR BOR®

B

21-Jun-2021 15:42:37

21 Jun 2021 15:41

Test passed

Operato RAA

Sample: FUEL A

Method: ISO 4406

Comment

Dilution: 0% (No multiplier)


For more information please visit: www.stanhope-seta.co.uk



Seta AvCount3


Laboratory Particle Counter for Fuel, Lubes and Hydraulic Oils

ASTM D7619; ATM D7647; ASTM D975; IP 565; Defence Standard 91-091; Defence Standard 91-86; IP PM FA; GOST 17216; ISO 4406; ISO 60970; NAS 1638; SAE 4059

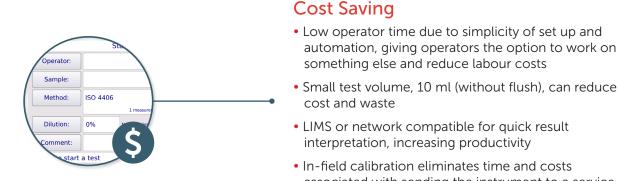

Ease Of Use

- Features simple user interface with touchscreen display
- The fully-automated test means extensive operator training is not required before using the instrument
- User-defined test methods are easily programmed



• Dilution protocol for testing of high viscosity samples

• Real-time display of test progress and ability to view

previous results whilst running a sample

 14 embedded methods for fuel and oil testing • User and sample identification - track and trace

Password-protected levels for security

associated with sending the instrument to a service

automation, giving operators the option to work on

something else and reduce labour costs

interpretation, increasing productivity


cost and waste

centre



Precision and Accuracy

- Fully automatic test sequence and consistent sample handling ensures test repeatability and reproducibility
- ISO 11171 calibration protocol
- Programmable alarm limits
- SQC analysis allows analysis of results in accordance with ASTM D6299



Enhanced Functionality

For more information please visit: www.stanhope-seta.co.uk



Seta AvCount3

Laboratory Particle Counter for Fuel, Lubes and Hydraulic Oils

ASTM D7619; ATM D7647; ASTM D975; IP 565; Defence Standard 91-091; Defence Standard 91-86; IP PM FA; GOST 17216; ISO 4406; ISO 60970; NAS 1638; SAE 4059

Operation			
Principle of operation	Laser obscuration		
Test methods	14 embedded test methods, user programmable		
	including ASTM D7619; IP 565; ISO 4406; NAS 1638; SAE 4059; GOST 17216		
Particle size range	ISO 11171: 4μ m(c) to 70 μ m(c) (calibration for larger sizes available on request		
Test duration	Less than 3 minutes		
Pressure (max)	Online pressure 10 bar gauge		
Sample temperature range	Ambient 0 to 70 °C		
Operating temperature range	Ambient 5 to 40 °C		
Relative humidity (max)	80% @ 40 °C		
Sampling method	Bottle sample and continuous		
	Size		
Programmable test method parameters (via PC)	Protocol (number of repeat measurements, flush volume before first measurement, flush volume between measurements, flush between measurements)		
	Single or automated repeat tests, interval between repeat tests		
Display and control system	Real time test progress and results, touchscreen		
Measurement			
Massuring channels	16 size channels displayed on instrument,		
Measuring channels	4μ m(c) to 70 μ m(c) and 2μ m to 100 μ m (ISO 4402 sizes)		
Counts per measurement (max)	60,000 per ml		
Coincidence error limit	60,000 particles/ml \geq 4µm(c) with \leq 5% co-incidence error (ISO 11171)		
Sample viscosity (max)	68 mm²/s (using internal pump), 200 mm²/s (pressure fed @ 3 bar gauge) (SA1950-0 Sample Delivery System is available as an accessory)		
Sample volume (typ)	80 ml for ASTM D7619 & IP 565, from 20 ml for other methods (includes flush cycles)		
Sample delivery	Integral Dual Piston Pump (DPS) downstream of the cell		
Sample flow rate	30 ml/min ±5 ml/min		
Data Management			
Results format	Cumulative, Particles/ml, ISO 4406 cleanliness codes/classes Numerical and graphical display		
Memory	500,000 result memory Print via internal printer, export to LIMS, USB or QR code		
Connectivity	RJ45 Ethernet or USB		
Number of calibration points	16 (MTD)		
Power requirements			
Voltage	100/240 V, 50/60 Hz, Auto-sensing universal power supply		
Physical			
Size (HxWxD) / Weight	370 x 230 x 270 mm / 6 kg		